

5351-5361

Caremor Cliner



CUSTOMER INSTRUCTIONS

PLEASE READ AND FAMILIARIZE YOURSELF WITH ALL INSTRUCTIONS BEFORE USING THIS PRODUCT. If you have trouble understanding these instructions contact your dealer or Winco customer support, (800) 237-3377 before attempting to use this product; otherwise injury may occur.

Winco assumes no responsibility for damage or injury caused by improper assembly, installation, use, or maintenance of these products.



1. READ AND FOLLOW ALL DIRECTIONS.
2. NEVER use tray as a restraint.
3. ALWAYS fold footplate up before user enters or exits the chair; otherwise INJURY MAY RESULT.
4. DO NOT stand on plastic footplate; INJURY MAY RESULT.
5. Keep users hands and feet clear of any moving parts. Attendant MUST confirm that users hands and feet are clear of moving parts before and while adjusting positions on tray or footrest or INJURY MAY RESULT.
6. Never use the chair arms or tray as a seat; INJURY MAY OCCUR.
7. Lock casters at all times, except when transporting chair.
8. Chair must ALWAYS be positioned on a level surface.
9. DO NOT use chair for Transporting in or with ANY type of vehicle or trailer. Winco chairs have not been tested or approved for use by an occupant in any type of vehicle or trailer.
10. Immediately remove from service; Any chair with broken parts, torn upholstery, or other mechanical or visible damage.
11. Periodically, recheck tightness of all nuts, bolts and screws.
12. USE ONLY WINCO AUTHORIZED REPLACEMENT PARTS.
13. NEVER EXCEED the recommended **weight capacity of 300 lbs.** (136 kg).
14. SAVE THESE INSTRUCTIONS for future reference and training.

5351-5361 Weight Capacity = 300 lbs. (136 kg.)

No Tools required for standard assembly.

PLEASE READ AND FAMILIARIZE YOURSELF WITH ALL INSTRUCTIONS BEFORE PROCEEDING WITH ASSEMBLY

Install the Back

1. After checking your product for any shipping damage, put chair in upright position.
2. Slide the **Back Frame** over the **7/8"** tubes of the **Seat Frame**. (FIG.3)
3. Depress the **1/4"** **Lock Button** in **Seat Frame** while pushing down on one side of **Back Frame**.
4. Repeat procedure on opposite side until both **Lock Buttons** are snapped into corresponding holes of **Back Frame**. **NOTE: Snap buttons must protrude out of holes on back frame. (FIG.4)**

WARNING: Failure to lock back and seat frames together may cause injury.

5. **Remove the wood spacing block from back frame after chair assembly.**
6. Press the "Hook & Loop" pieces together on bottom of chair back, to complete assembly and give finished look to back of chair.

Operation of the Tray – 5351 Only

7. The **Tray** automatically locks into the first position; depress the **Latch Button** for 2 more positions.
8. The **Right Tray Arm** is movable to compensate for minor variations in the width of the chair.
9. Storing the **Tray**; Insert the left tray arm tube into the right tray receiving tube and the **Latch Button** will lock it into place. Allow the right side of the table to hang down vertically on the right side of chair (Left & Right; as if you are seated in chair).
10. To make the tray permanently non-locking, remove the **Snap Button** of the **Right Tray Arm**.

Operation of the Chair

There are two ways to operate this chair; Attendant Controlled & User Controlled.

11. The chair comes from the factory set up for Attendant Controlled positioning of the chair. This means the Release Handle must be actuated by an attendant before positioning of the chair can be changed. By squeezing the Release Handle – moving the chair to the desired position – and releasing the handle - the attendant can position the patient in an infinite number of positions. **(FIG.2)**

NOTE: The attendant must also squeeze the handle to allow the patient to be brought back to the standard sitting position before the patient can get out of the chair safely.

12. The chair can be changed from the Attendant positioning to User Controlled positioning. This means that the Release Handle must be relocated underneath the left Upholstered Armrest (the instructions on the following pages will describe how you can make this change to your chair). Once this change is made, the User can control their own recline position by squeezing the handle under the left Upholstered Arm of the chair. **(FIG.1)**

NOTE: The attendant can still operate the chair; however, leverage to move the patient will not be as effective as with the Attendant Controlled positioning option.



WARNING

*Stay clear of recline mechanism.
Periodically recheck tightness of ALL screws & bolts, & never use the tray as a restraint.*

Maintenance of the Chair

13. To ensure proper operation of the reclining mechanism, lubricate all pivot points with a silicone lubricant at least twice yearly.
14. The back cushion can be replaced by opening the “Hook & Loop” flap on the lower rear of the back cushion, removing the Push Handle, and sliding it off of the **Back Frame**. **(FIG.3)**
15. The seat/legrest cushion can be replaced by removing the (2) seat hold-down slat screws (attaching the underside-rear of the seat cushion to the chair frame) then slide the cushion off toward front of chair.


Optional 5-inch Caster Placement

16. The casters on this 5351-5361 chair, can be configured one of two ways; Rigid casters in front & Total Lock casters on rear or vice versa.

If you wish your chair to have casters in opposite configuration, please follow below instructions.

- a) Lay chair on side on carpeted surface. Use a Phillips screwdriver and 7/16” wrench to remove the 1/4” bolt & nut from chair legs.
- b) Remove bolts and casters. IMPORTANT: Be sure to also remove the plastic Caster Insert Sleeve from chair leg. This piece must be repositioned so that the bolts line up with slot on Insert Sleeve when caster is re-inserted into chair leg.
- c) Re-insert casters into chair legs. (Follow IMPORTANT note in above step)
- d) Insert bolts and nuts; tighten all with screwdriver and wrench.




Wrinkles in Vinyl – Storage and shipping can cause wrinkles of the vinyl on your Winco chair. This is normal. Please allow 1-2 weeks at room temperature (approx. 70 degrees) to allow for vinyl to expand back to original appearance.

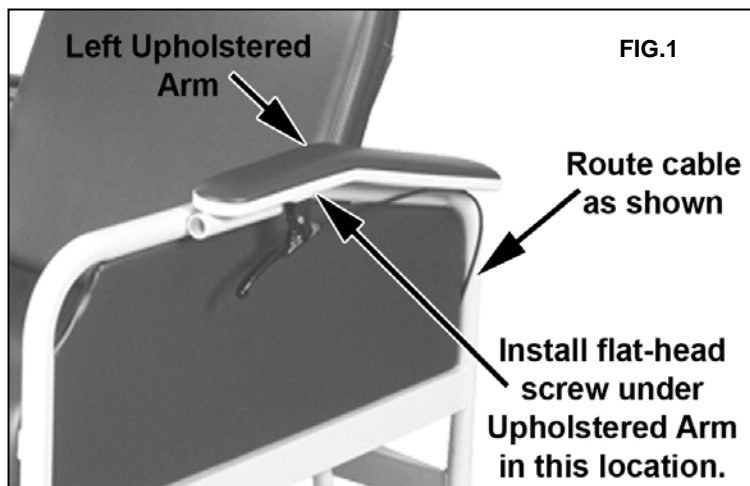

Optional Release Handle Mounting location:

Tools Needed: Phillips Screwdriver & Flat Screwdriver

1. Use Phillips screwdriver & remove the Release Lever and screw from the Push Handle.
2. Use Phillips screwdriver & remove the rear screw that attaches rear of left Side Panel.
3. Use flat screwdriver & remove left Armrest, and then insert the included flat-head screw into hole with countersink located on metal arm plate.
4. Route the Release Lever between the Side Panel and Frame as shown in photo above.
5. Use flat screwdriver & thread flat-head screw into the Release Lever and tighten.
6. Re-install Armrest.
7. Re-attach rear of Side Panel.
8. Install the included plastic "Split-Stem Cap" in the empty hole on the Push Handle.

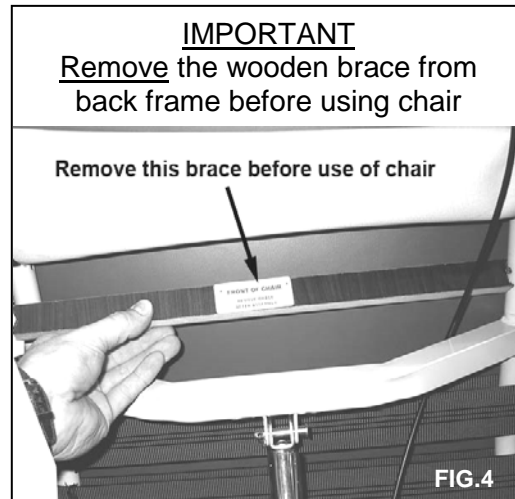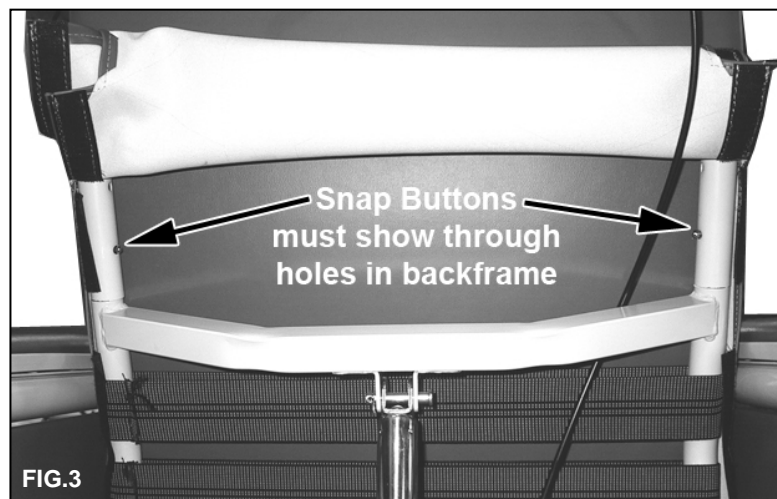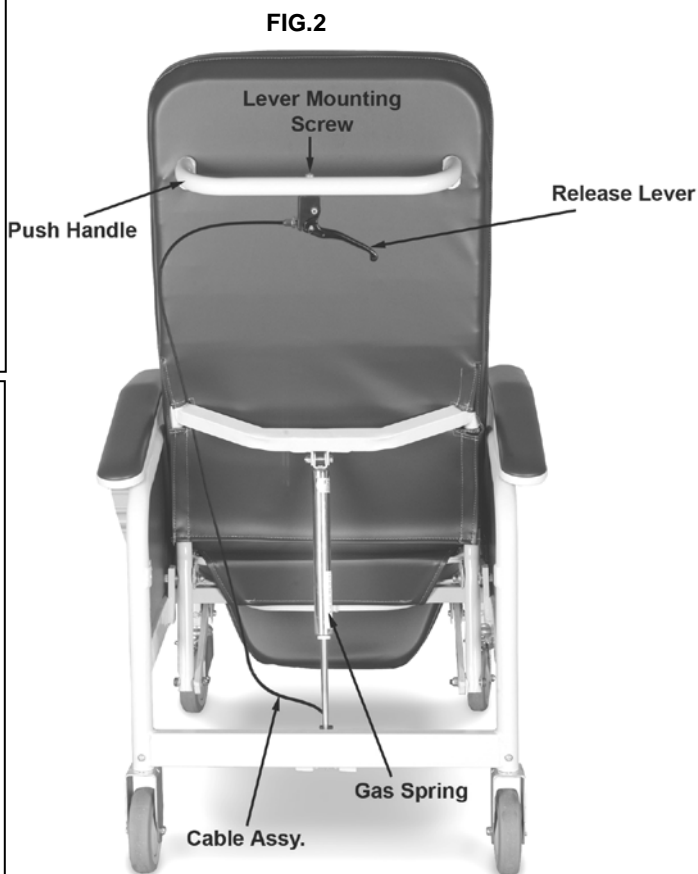

Visit our website www.wincomfg.com/product-documents/parts-lists for a complete parts list catalog of your chair or call Customer Service @ 1-800-237-3377 to request it by mail.

GENERAL CARE & CLEANING:

- REGULARLY lubricate pivot points on the recline mechanism with a lubricant approved by your facility. Periodically position the chair back into full recline position to keep the gas cylinder lubricated.
- Periodically inspect tightness of all screws, bolts, and nuts.

Winco furnishings are built to provide durable reliable service when properly cared for.

In general all of our products should be 1) Cleaned 2) Rinsed 3) Allowed to air dry.

It is important to note that disinfecting a product is not the same as cleaning the product. Disinfectants alone will not provide adequate cleaning, they do not have grease or oil cutting properties to remove grime or hair and skin oils. Over time, the appearance and feel and performance of your upholstery may diminish if not cleaned properly

CLEANING:

Remove grime, hair and body oils; Your furnishings should be cleaned with mild soap & water solution and a damp cloth on a regular basis (especially where skin & hair make contact with upholstery). Avoid harsh detergents or chemicals that could damage the upholstery or finish of your recliner. If the furnishing is disinfected with chemicals or bleach, it MUST be wiped off using only clean water on a damp cloth and then be allowed to air dry. Failure to rinse upholstery with clean water can result in a build-up of residues over time that can dry out the upholstery and cause changes to the look and feel of the upholstery and eventually can lead to cracking.

FOR FURTHER CLEANING INFORMATION on standard Winco vinyl's VISIT:

<http://spradlingvinyl.com/asset/docs/research/ApprovedCleaners.pdf>

<http://spradlingvinyl.com/asset/docs/research/CompleteCareandCleaningGuides.pdf>

Other Quality Winco Medical Furnishings You May Be Interested In:



Clinical
Recliners




Exam Tables



Convalescent (LTC)
Recliners



Ring Binder
Carts

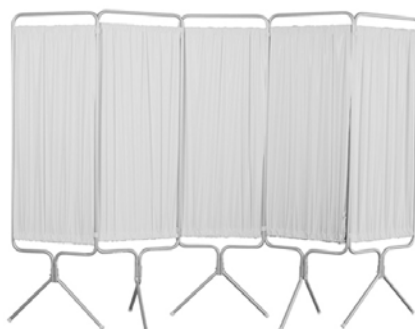

Privacy Screens



Phlebotomy
Chairs



Specialty Chair
Transfer Chairs



Stools



Room Chairs

Visit us online at www.wincomfg.com

Products with the following markings are intended for commercial use only.



(MDD 93/42/ECC
MDSS GmbH
Burckhardtstr. 1
D-30163 Hannover
Germany



100-240 VAC 44W, 50-60Hz

Supply: 12V

IP XX

Operating Conditions:

10° - 40° C

WARNING: Long-term, continuous exposure to heat may cause burns. Read instructions before using. DO NOT use wet. DO NOT insert pins into upholstery.

SYMBOLS



Visit our website www.wincomfg.com/product-documents/parts-lists for a complete parts list catalog of your chair or call Customer Service @ 1-800-237-3377 to request it by mail.



ISO 9001-2008 CERTIFIED



LIMITED WARRANTY

• 5516 SW 1st Lane • Ocala, FL 34474
 • Phone (352) 854-2929 • (800) 237-3377
 • Fax (352) 854-9544
 • www.wincomfg.com
 • customerservice@wincomfg.com

TERMS

Winco Mfg., LLC. warrants this product to be free of manufacturer's defects in material and workmanship, provided that the product is used according to normal operating conditions and proper maintenance intended by manufacturer. This warranty is available only to the original retail purchaser, is non-transferable and commences on the date of retail sale; proof of purchase required.

Limited One Year Product Warranty: Winco Mfg., LLC warrants the complete product for one (1) year. At Winco Mfg., LLC. sole discretion, it may repair or replace any components freight free that are found to be defective during the first year. *Winco Mfg., LLC. shall not be liable for any labor, or any other costs incurred as a result of or in conjunction with a warranty claim.*

Limited Three Year Warranty: Winco Mfg., LLC warrants recliner mechanisms, electrical components, vinyl panels and Vinyl on upholstered parts [from cracking or delaminating] pressurized gas springs, and casters, when new, for a period of three (3) years. At Winco Mfg., LLC. 's Sole discretion, it may repair or replace components found to be defective. *Winco Mfg., LLC. shall not be liable for any labor, shipping or any other costs incurred as a result of or in conjunction with a warranty claim.*

Limited Lifetime Frame Warranty: Winco Mfg., LLC warrants steel and aluminum base frames for all products, when new, for the lifetime of the original purchaser. This limited warranty does not apply to paint/finish or any components attached to the frame such as; upholstery, foam, casters, mechanisms or related parts that are covered under above warranties. *Winco Mfg., LLC shall not be liable for any labor, shipping or any other costs incurred as a result of or in conjunction with a warranty claim.*

The purchaser's exclusive remedy under this warranty shall be limited to such repair or replacement of defective components at Winco Mfg., LLC sole discretion. For warranty service, contact the dealer that the product was originally purchased from or Winco Mfg., LLC directly.

EXCLUSIONS

There are no other warranties, conditions, representations or guarantees, express or implied, made or intended by Winco Mfg., LLC and all other warranties, conditions, representations or guarantees including any warranties, conditions, representations or guarantees under any Sale of Good Act or Like legislation or statute is hereby expressly excluded. Any and all other implied warranties shall not extend beyond the duration of the express warranty. Liability for incidental or consequential damages is excluded to the extent permitted by law. Some states do not allow the exclusion or limitation so the above limitation or exclusion may not apply to you. This warranty gives you specific legal rights. In addition you may also have other rights, which vary from state to state.

GENERAL PROVISIONS

No warranty herein contained or set out shall apply when damage or repair is caused by any of the following:

1. Damage in transit.
2. Accident, alteration, abuse or misuse of product i.e. exceeding weight capacities, applying inordinate pressure to footrest/leg rest, use in Mental Health facilities like institutions or, any unintended use of the product or use in unintended environments (i.e. outdoor, showers, MRI rooms, etc.)
3. Fire, water damage, theft, war, riot, hostility, acts of God.

Examples contained in this list are not to be construed as all-inclusive.



Design, appearance, parts, & construction are subject to change without notice